


User Prabakaran Thiru

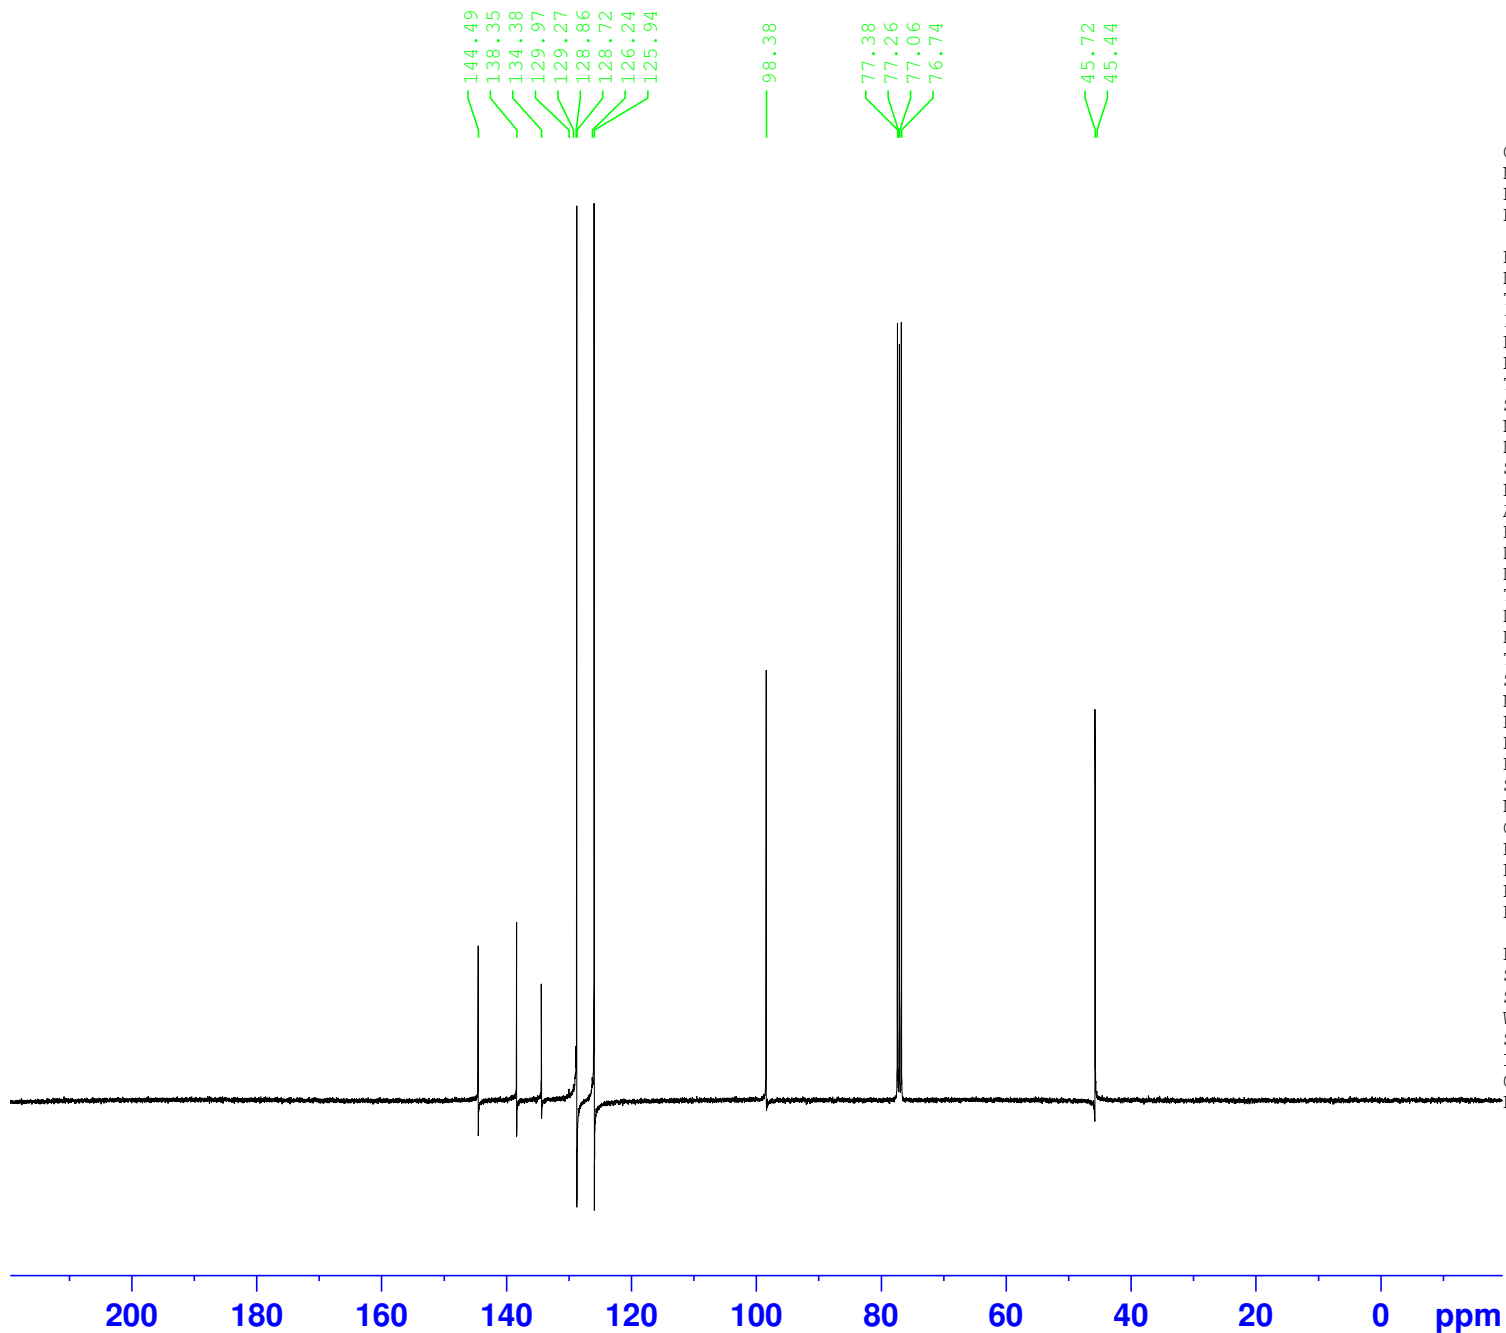

Current Data Parameters  
NAME 05092025-prathch-237-1  
EXPNO 2  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20250905  
Time 19.04 h  
INSTRUM AVIIHD400  
PROBHD Z122623\_0022 (   
PULPROG zgpg30  
TD 65536  
SOLVENT CDCl3  
NS 256  
DS 4  
SWH 24038.461 Hz  
FIDRES 0.733596 Hz  
AQ 1.3631488 sec  
RG 177.9  
DW 20.800 usec  
DE 18.00 usec  
TE 295.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 100.6228289 MHz  
NUC1 13C  
P0 3.17 usec  
P1 9.50 usec  
PLW1 39.00000000 W  
SFO2 400.1316005 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 8.80000019 W  
PLW12 0.13265000 W  
PLW13 0.06672400 W

F2 - Processing parameters  
SI 32768  
SF 100.6127685 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40