


User Christoph Gross

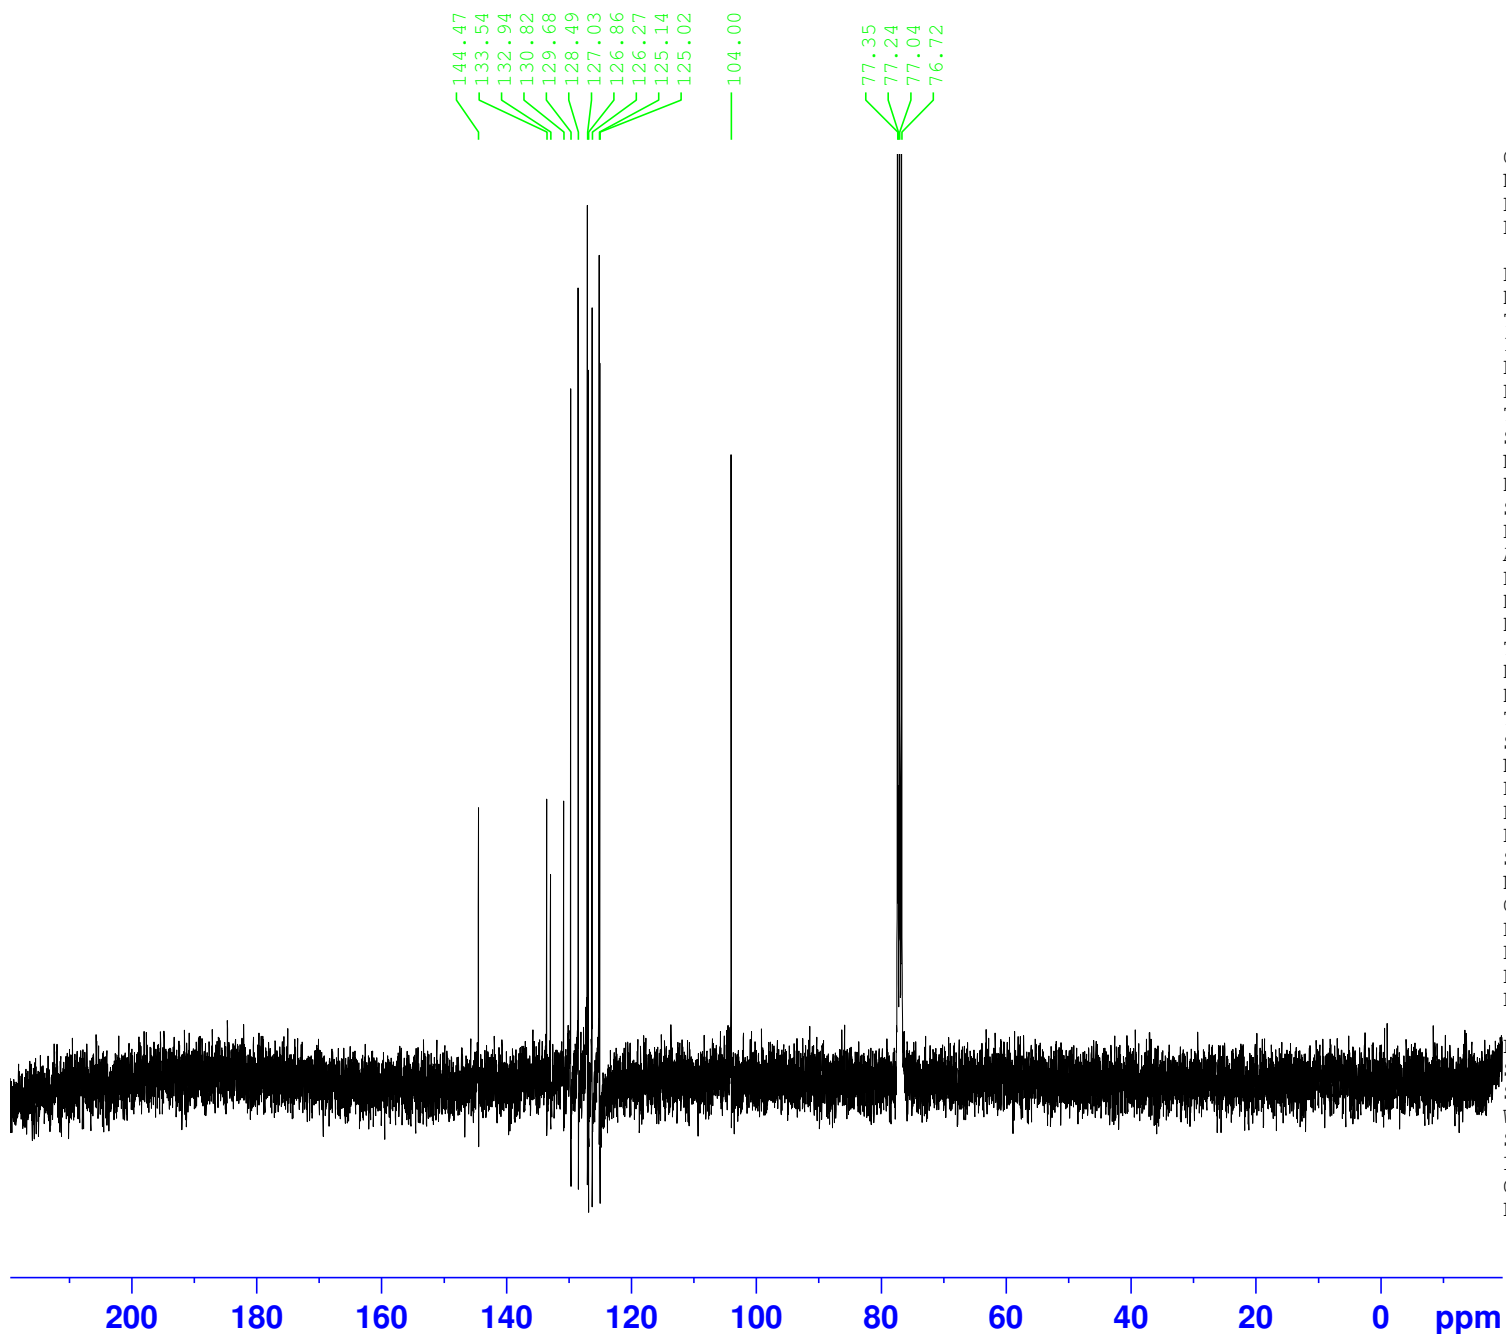

Current Data Parameters
NAME CG743
EXPNO 2
PROCNO 1

F2 - Acquisition Parameters
Date_ 20250221
Time 15.14 h
INSTRUM AVIHD400
PROBHD Z122623_0022 (
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 128
DS 4
SWH 24038.461 Hz
FIDRES 0.733596 Hz
AQ 1.3631488 sec
RG 198.74
DW 20.800 usec
DE 18.00 usec
TE 295.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 100.6228289 MHz
NUC1 13C
P0 3.17 usec
P1 9.50 usec
PLW1 39.00000000 W
SFO2 400.1316005 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 8.80000019 W
PLW12 0.13265000 W
PLW13 0.06672400 W

F2 - Processing parameters
SI 32768
SF 100.6127685 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40